



Glooko[®] Uploader

Instructions for use – for Glooko users

Contents

Find your device	4-5
General information	6
Product description.....	6
Intended use.....	6
Supported devices.....	6
Warnings.....	6
Contraindications	6
Instructions for use	7
Patients	8
Sign into your MyGlooko dashboard at https://my.glooko.com	8
Download the software installation file	8
Locate the installation file and run the file.....	8
Healthcare providers.....	9
Request a link to download the Glooko Uploader software.....	9
Download the software installation file	9
Locate the installation file and run the file.....	9
Patients and healthcare providers	10
Open the Glooko Uploader software.....	10
Sign into your Glooko account.....	10
Features in Glooko Uploader	11
Upload diabetes data	12
View diabetes data.....	13
Compatible devices and transmission methods	14

Find your device



Glucose meter



CGM



Insulin pump

Abbott

FreeStyle Freedom Lite.....	14
FreeStyle InsuLinx	14
FreeStyle Lite.....	14
FreeStyle Optium Neo.....	14
FreeStyle Precision Neo.....	14
Precision Xtra	14
Precision Xceed.....	14

Acon Laboratories

On Call® Express.....	14
On Call® Express II.....	14
On Call® Express Voice	14

AgaMatrix

WaveSense Jazz™	14
-----------------------	----

Animas

OneTouch Ping (meter)	14
-----------------------------	----

Animas

OneTouch Ping (pump).....	17
Vibe	17

Arkray

GlucoCard Shine Connex	14
GlucoCard Shine Express	14
GlucoCard Shine XL	14
ReliOn Premier Blu.....	14
ReliOn Premier Classic.....	14
ReliOn Premier Voice.....	14

Ascensia (Bayer)

Breeze 2	15
Contour.....	15
Contour Care.....	15
Contour Fit.....	15
Contour Link	15
Contour Next.....	15
Contour Next (Bluetooth)	15
Contour Next One.....	15
Contour Plus	15
Contour Plus One.....	15
Contour next EZ	15
Contour next Link.....	15
Contour next Link 2.4	15
Contour next USB.....	15
Contour TS.....	15
Contour XT	15
Contour USB.....	15

Dexcom

G4 Platinum.....	17
G4 Platinum with Share.....	17
G5.....	17
Touchscreen Receiver (G5).....	17

GlucoRx

Nexus.....	15
Q.....	15


i-SENS

alphacheck professional	15
CareSens BGM/TEE2	15
CareSens N	15
CareSens N POP.....	15
CareSens N Voice.....	15


Insulet

Omnipod®.....	18
Omnipod® Dash™ System	18


Intuity

 POGO® Automatic™	15
--	----


LifeScan

 OneTouch Select Plus	15
OneTouch Ultra	15
OneTouch Ultra2	15
OneTouch UltraEasy	15
OneTouch UltraMini	15
OneTouch Verio	15
OneTouch Verio Flex	15
OneTouch Verio IQ	15
OneTouch Verio Reflect	15
OneTouch Verio Sync	15


Medtronic

 630G	18
640G	18
670G	18


Menarini

 GlucoMen LX2	16
--	----

Prodigy



 AutoCode	16
--	----

Roche


 Accu-Chek Active	16
Accu-Chek Aviva Connect	16
Accu-Chek Aviva Combo	16
Accu-Chek Aviva Expert	16
Accu-Chek Aviva Insight	19
Accu-Chek Aviva Nano	16
Accu-Chek Aviva Plus Black	16
Accu-Chek Aviva Plus Silver	16
Accu-Chek Compact Plus	16
Accu-Chek Guide	16
Accu-Chek Guide Me	16
Accu-Chek Instant	16

Accu-Chek Mobile (USB)	16
Accu-Chek Nano	16
Accu-Chek Performa	16
Accu-Chek Performa Insight	19
Accu-Chek Performa Nano	16


Roche

 Accu-Chek Aviva Insight	19
 Accu-Chek Performa Insight	19

Sanofi

 BGStar	16
--	----

Tandem

 t:flex	18
 t:slim	18
t:slim G4	18
t:slim X2	18

Trividia (Nipro)

 TRUE METRIX	16
TRUE METRIX AIR	16
TRUEresult	16
TRUEyou mini	16

General information

Product description

Glooko Uploader® is indicated for use by individuals or healthcare professionals in the home or healthcare facilities to transfer predefined data from home monitoring devices to a server database. The device can be used as a stand-alone product or in combination with the Glooko System.

Intended use

Glooko is a data management software intended for use in home and professional settings that assists individuals with diabetes and healthcare professionals in reviewing, analysing and evaluating device data in order to support an effective diabetes management programme. Glooko connects to compatible medical devices and trackers to allow users to transfer their data to the Glooko system. Glooko is not intended to provide treatment decisions or to be used as a substitute for professional healthcare advice.

Supported devices

To get started, individuals will need:

1. A compatible blood glucose meter, insulin pump or continuous glucose monitor (CGM);
2. A PC or Mac computer with one of the following operating systems (OS):
 - Windows 8.1 (32-bit and 64-bit)
 - Windows 10 (32-bit and 64-bit)
 - macOS 10.14: Mojave
 - macOS 10.15: Catalina
 - macOS 11.0: Big Sur
3. the Glooko Uploader software;
4. A Glooko account; and
5. The syncing or device download cable supplied with the supported diabetes device.

Warning!

Glooko does not measure, interpret, or make decisions on the data it conveys nor is it intended to provide automated treatment decisions or be used as a substitute for professional judgment. All medical diagnosis and treatment are to be performed under the supervision and oversight of an appropriate healthcare provider.

Contraindications


None.

Instructions for use – Glooko Uploader

You will need to create a Glooko account to use Glooko Uploader. The data uploaded using Glooko Uploader will synchronise to your Glooko account, which can be accessed using your Glooko login information. Internet (WiFi or mobile data network) access is necessary for your data to synchronise to the Glooko server.

Patients:

- Learn how to install and upload data using Glooko Uploader on the next page.

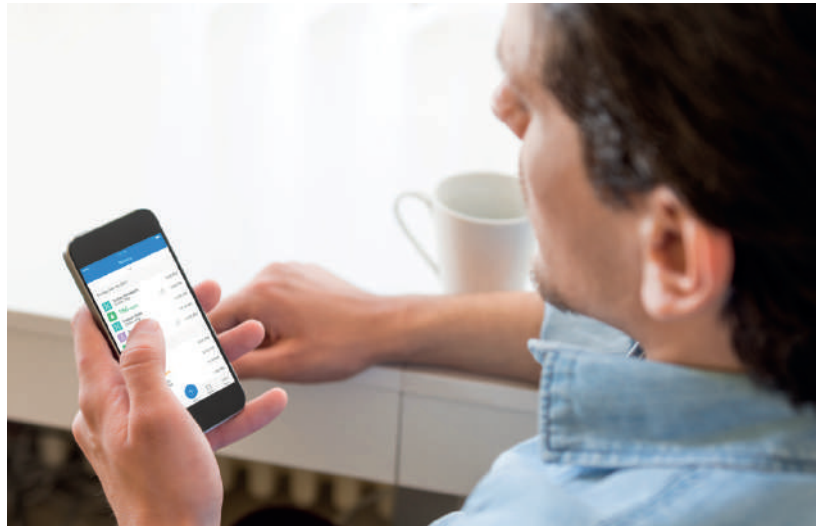

Healthcare providers:

- Learn how to install and upload data using the Glooko Uploader on page 9.



Patients


In order to access the MyGlooko dashboard and download the Glooko Uploader software, you will need to have a Glooko account. You can sign up for Glooko using the Glooko mobile app for iOS or Android. You can also contact **Glooko Support** (<https://support.glooko.com>) for assistance in creating an account. Once you have created a Glooko account, please follow the instructions below.

1 Sign into your MyGlooko dashboard at <https://my.glooko.com>

- Enter your email address and password.
- Tap Sign In.

GET HELP SIGNING INTO YOUR GLOOKO ACCOUNT

- **FORGOT PASSWORD:**
If you are unable to remember your password to sign in, tap **Forgot Password** to receive a password reset email. Follow the instructions on the screen. You can also contact Glooko Support for assistance.
- **UNLOCK YOUR ACCOUNT:**
If you enter your password incorrectly five times, your account will be locked. An email with unlock instructions will automatically be sent to the email address registered to your account. However, if you do not receive an email, click **Didn't receive unlock instructions** – you will be redirected to the Unlock page. Follow the instructions on the screen. You can also contact Glooko Support for assistance.

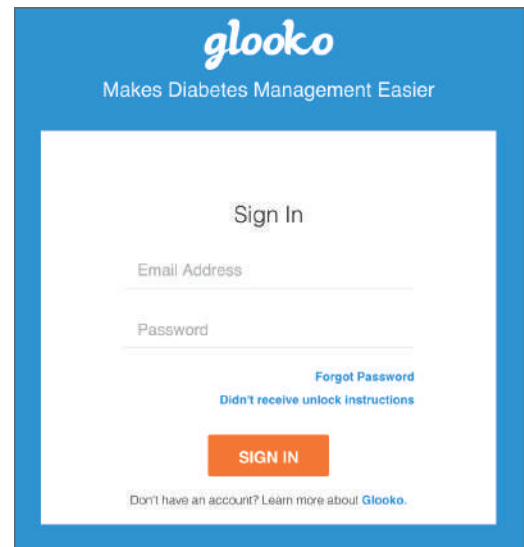

2 Download the software installation file

After logging into your MyGlooko dashboard, you will need to download the installation file.

- Tap **Settings**.
- Scroll to the bottom of the page and click **Get Glooko Uploader**.
- You will be taken to a screen with buttons to install Glooko Uploader on a Mac or PC. Click either the Mac or PC button to download the installation file.



3 Locate the installation file and run the file

Depending on your web browser and operating system, you may need to search for the downloaded installation file or you may see a popup window asking you to run the file.

- If you are using a **PC**, look in your recent downloads folder
- If you are using a **Mac**, look in the downloads folder in Finder

Once you have located the file, double-click on it and follow the installation instructions on the screen.
NOTE: You will need to restart your computer at the end of the installation process.

Healthcare providers

In order to use the Glooko Uploader software, you will need a Glooko provider account and a subscription that supports Glooko Uploader. You will also need a specific link to download Glooko Uploader. Please contact Glooko Support (<https://support.glooko.com>) for assistance.

1 Request a link to download the Glooko Uploader software

Healthcare providers must request a link to download the Glooko Uploader software.

- Please contact Glooko Support (<https://support.glooko.com>) to request a link to download the Glooko Uploader software.

2 Download the software installation file

- When you receive the link to download the software from Glooko, click the link in your email. You will be taken to a screen with buttons to install Glooko Uploader on a Mac or PC. Click either the Mac or PC button to download the installation file.



3 Locate the installation file and run the file

Depending on your web browser and operating system, you may need to search for the downloaded installation file or you may see a popup window asking you to run the file.

- If you are using a **PC**, look in your recent downloads folder
- If you are using a **Mac**, look in the downloads folder in Finder

Once you have located the file, double-click on it and follow the installation instructions on the screen.

NOTE: You will need to restart your computer at the end of the installation process.

Patients and healthcare providers

After installing Glooko Uploader (Instructions for patients; Instructions for healthcare providers) and restarting your computer, locate the Glooko Uploader icon on either your desktop (PC) or in your Applications folder (Mac).

4 Open the Glooko Uploader software

- **Locate** the Glooko Uploader icon on your desktop (PC) or in your Applications folder (Mac).
- **Double-click** on the Glooko Uploader icon to start the program.

NOTE: Make sure you have restarted your computer before starting Glooko Uploader for the first time.



5 Sign into your Glooko account

Once the Glooko Uploader program opens, you will need to sign into your Glooko account.

- Enter your **email or username**
- Enter your **password**
- Tap **Sign In**.

GET HELP SIGNING INTO YOUR GLOOKO ACCOUNT


If you cannot remember your password to sign in, click **Forgot Password** to receive a password reset email. You can also contact Glooko Support for assistance.

A screenshot of the Glooko Uploader application window. The window title is 'Glooko Uploader'. The main heading is 'SIGN IN'. Below this is a message: 'To upload data, please sign into your Glooko account.' followed by 'Don't have an account?' and two links: 'Patients: Sign Up.' and 'Clinics: Contact Glooko Support.' There are two input fields: 'Email or Username' and 'Password'. Below the password field is a link 'Forgot Password?'. At the bottom is a blue 'Sign In' button. The footer says '©2018 Glooko Inc.'.


Patients and healthcare providers


6 Features in Glooko Uploader

LOG OUT OF YOUR ACCOUNT


- You can log out of your Glooko account by tapping the Profile button  in the bottom right-hand corner of Glooko Uploader.
- Tap **Log out**


VIEW YOUR PROFILE INFORMATION

- You can view your profile information by tapping the Profile button  in the bottom right-hand corner of Glooko Uploader.
- This popup includes:
 - o Your **name**
 - o Your **primary authorised site** (healthcare provider) and the associated **ProConnect code**
 - o Your **email address**
- Tap **Log Out**.

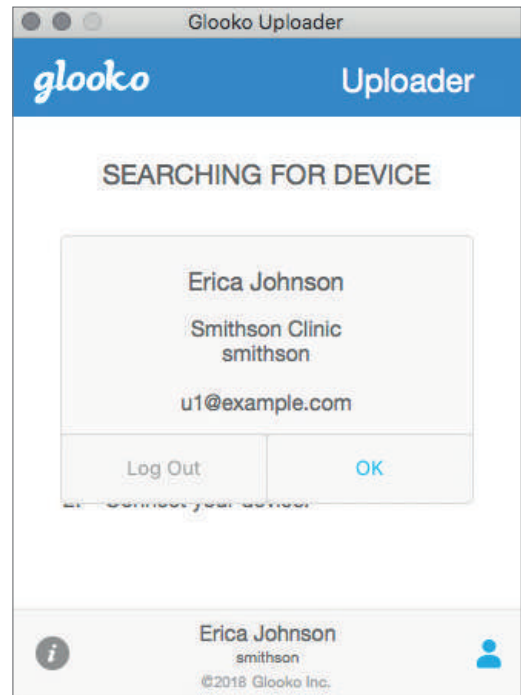

SEE ADDITIONAL INFORMATION ABOUT GLOOKO UPLOADER

- You can view additional information by tapping the Info button  in the bottom left-hand corner of Glooko Uploader.
- This popup includes product support information, product description, and the intended use statement.

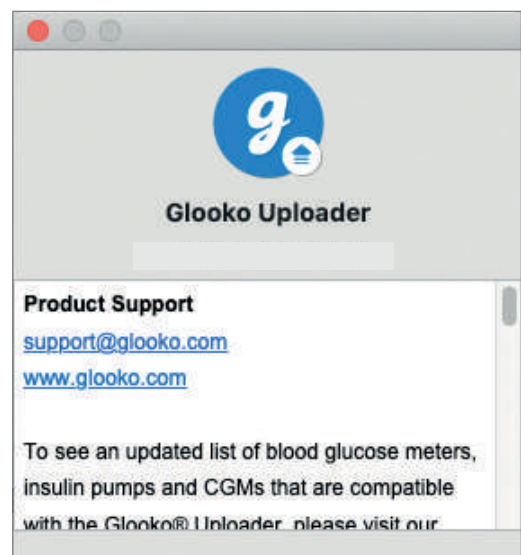

Patients and healthcare providers


7 Upload diabetes data

Once you have signed into Glooko Uploader, you can upload your diabetes device data.

CONNECT THE CABLE FOR YOUR DIABETES DEVICE TO THE COMPUTER

After logging in, Glooko Uploader will start searching for a device.

- Connect the appropriate USB cable or infrared (IR) cable for the diabetes device to the computer.
- Once the cable is recognised, wait a few seconds for the cable drivers to be recognised before connecting your device.

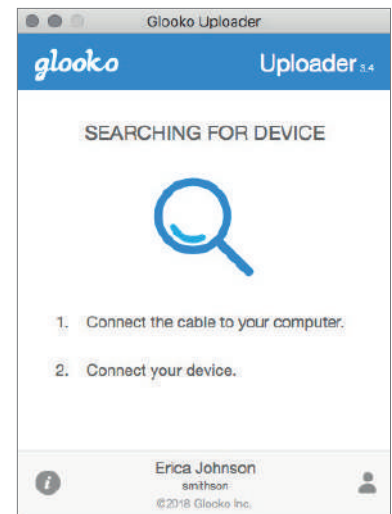


CONNECT THE DIABETES DEVICE TO THE CABLE

- After connecting the cable to the computer, connect the diabetes device to the cable.
- Click here to learn more about what cable you need to upload your diabetes device.

NOTE: Make sure you use the cable supplied with your diabetes device. If you need a new cable, please contact the manufacturer of your diabetes device.

- After connecting the diabetes device to your computer using the cable supplied with the device, your device will begin uploading data using Glooko Uploader.
- If an error occurs, please follow the instructions on the screen to resolve the error. If you continue to experience difficulties, please contact Glooko Support for assistance.

NOTE: The first time you upload data from your device, you may be asked to validate your user account. If prompted, please enter your username and password to complete the upload and assign the device to your account.

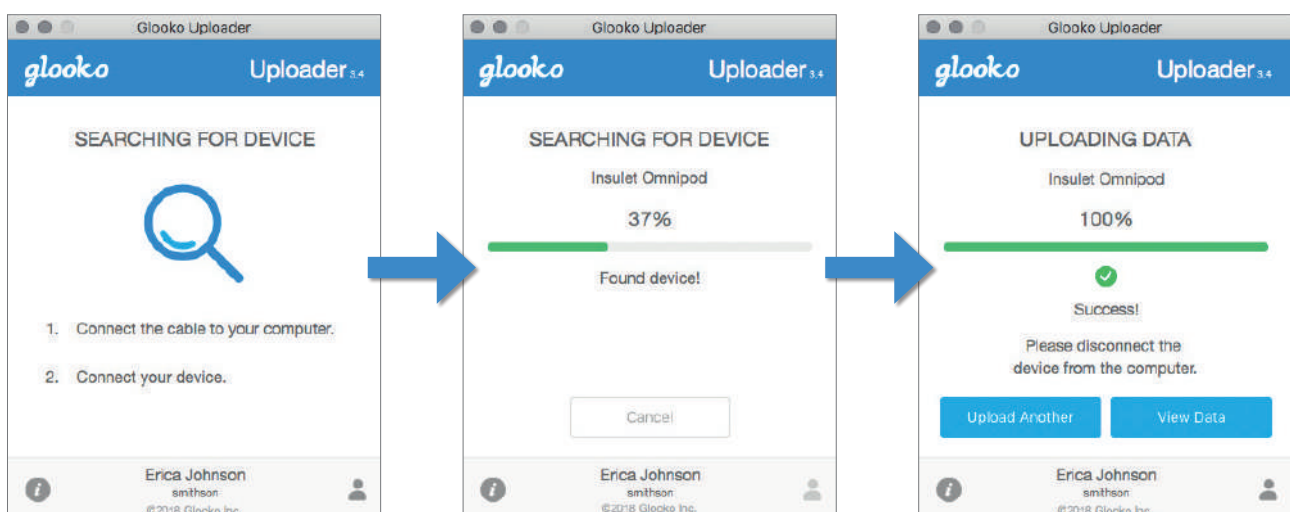

Patients and healthcare providers

8 View diabetes data


After uploading your diabetes device data using Glooko Uploader, you can view the data at <https://my.glooko.com> by logging into your Glooko account.

- **Patients:**
To learn more about the MyGlooko web dashboard, please refer to [Glooko for personal use – Quick start guide](#) at <https://support.glooko.com>
- **Healthcare providers:**
To learn more about Population Tracker, please refer to: [Glooko for clinics – Quick start guide](#) at <https://support.glooko.com>




Compatible devices and transmission methods


Below are instructions on how to upload diabetes data to Glooko using diasend® Uploader. Unless explicit upload instructions are provided for the device, it will upload automatically when you connect it to the PC/Mac using its specific USB cable.

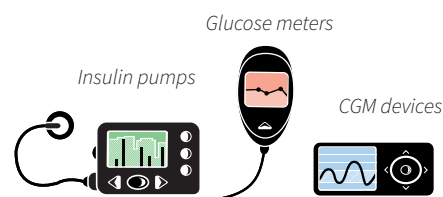


Blood glucose meters – connected via USB cable

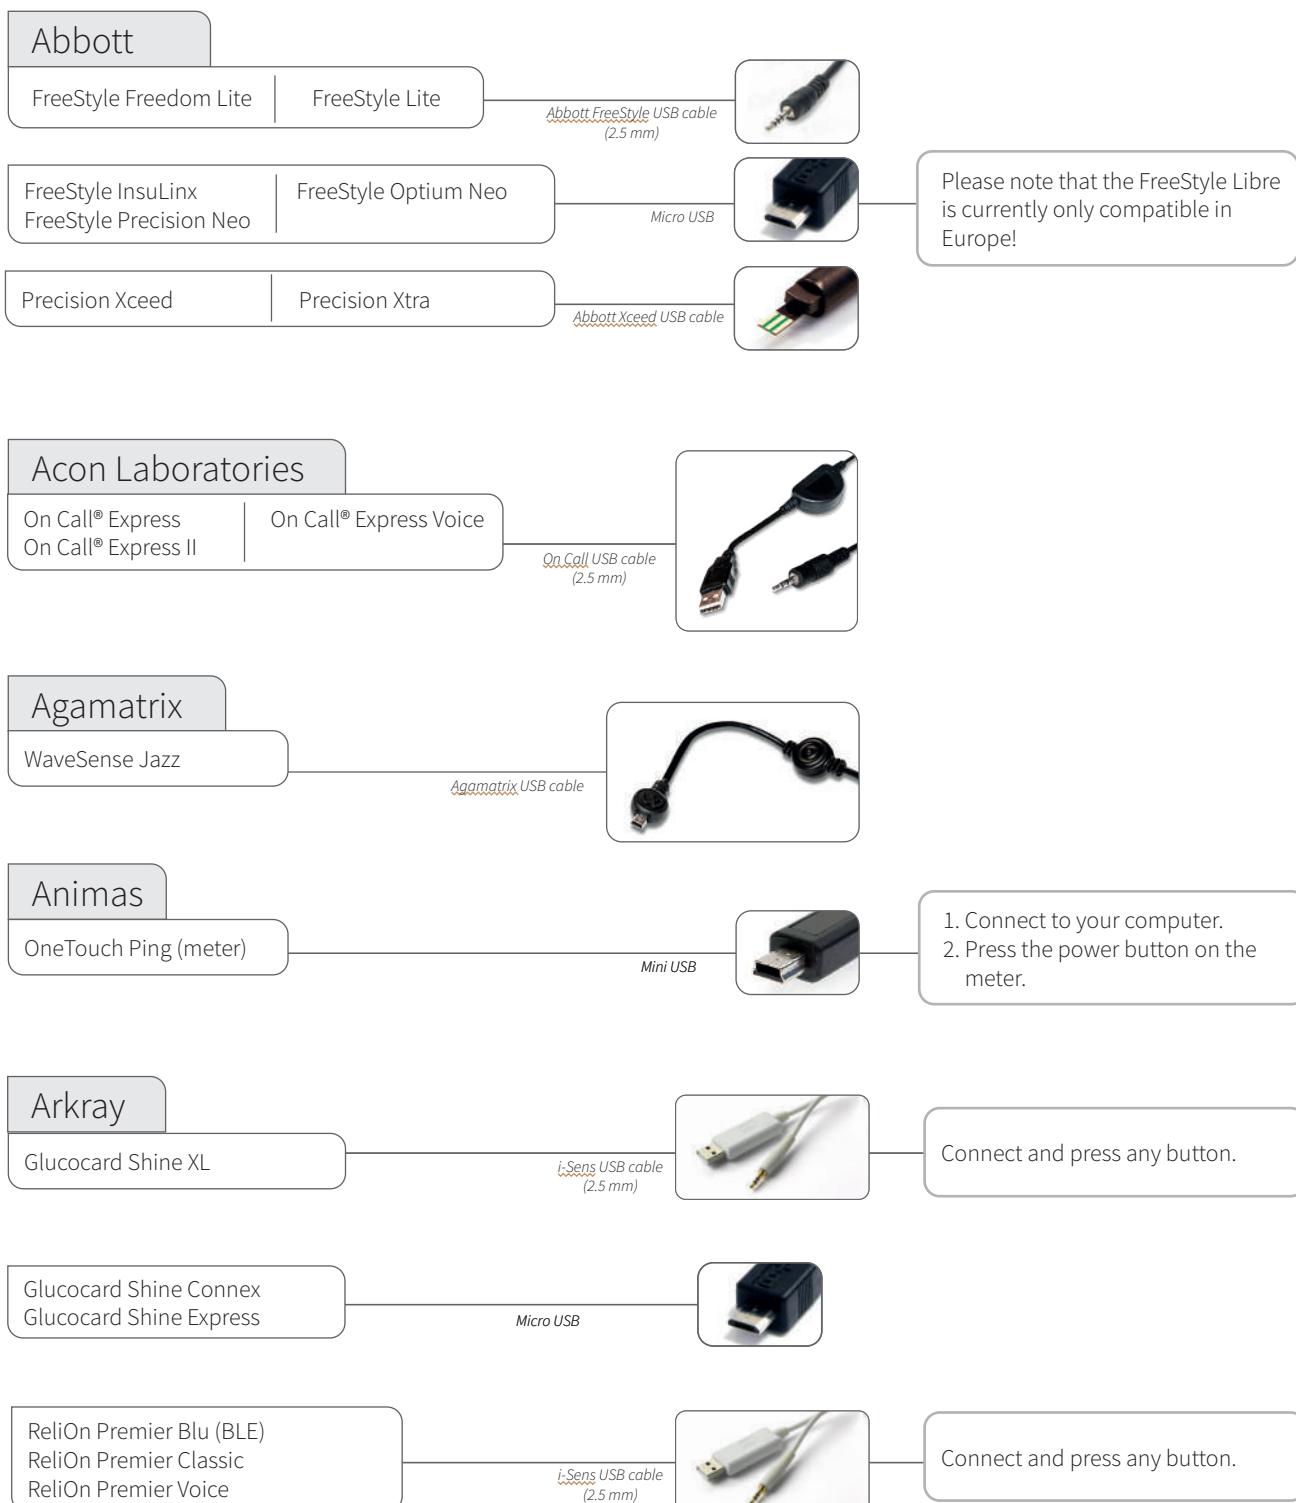


Blood glucose meters – connected via USB cable

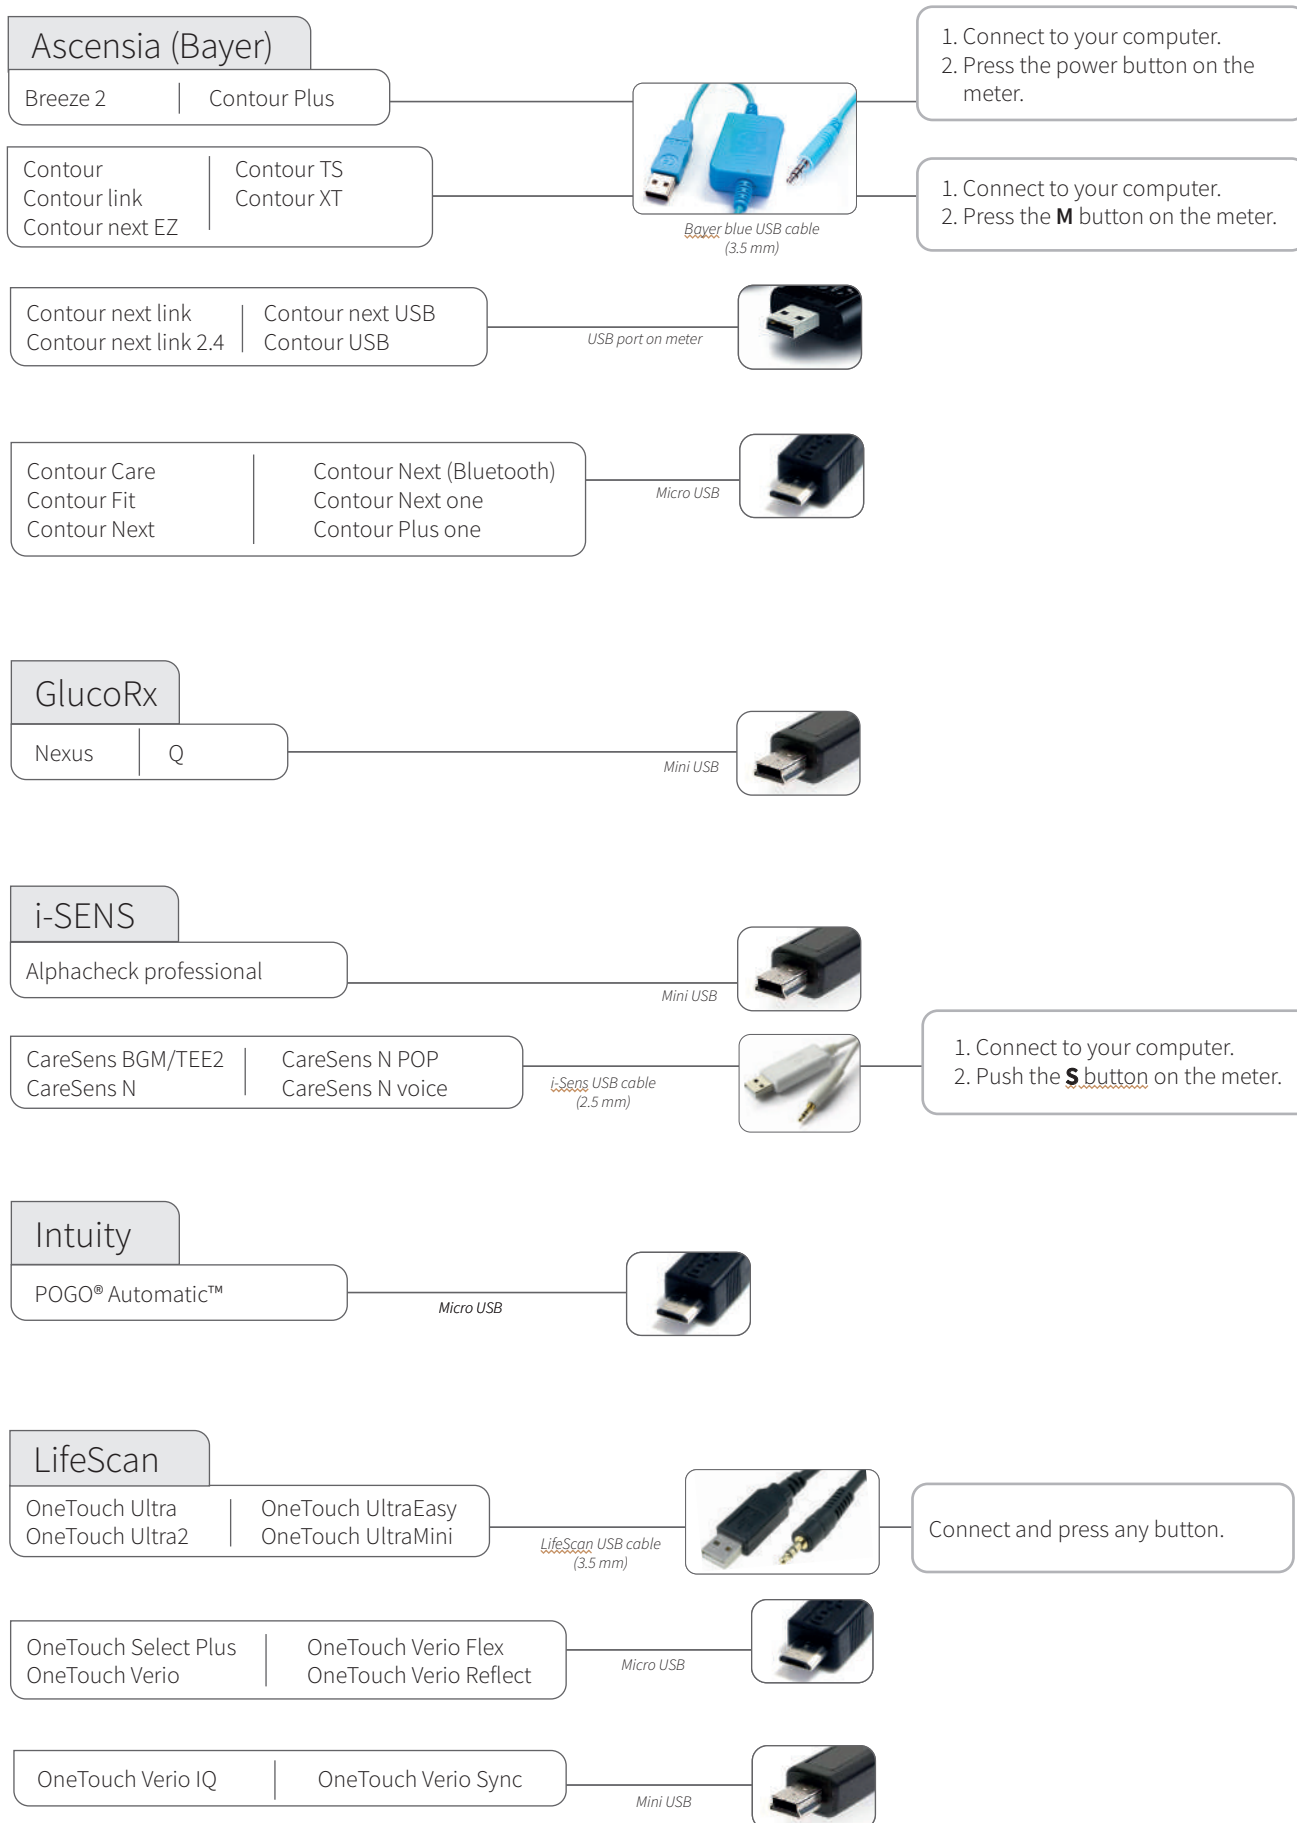


Blood glucose meters – connected via USB cable

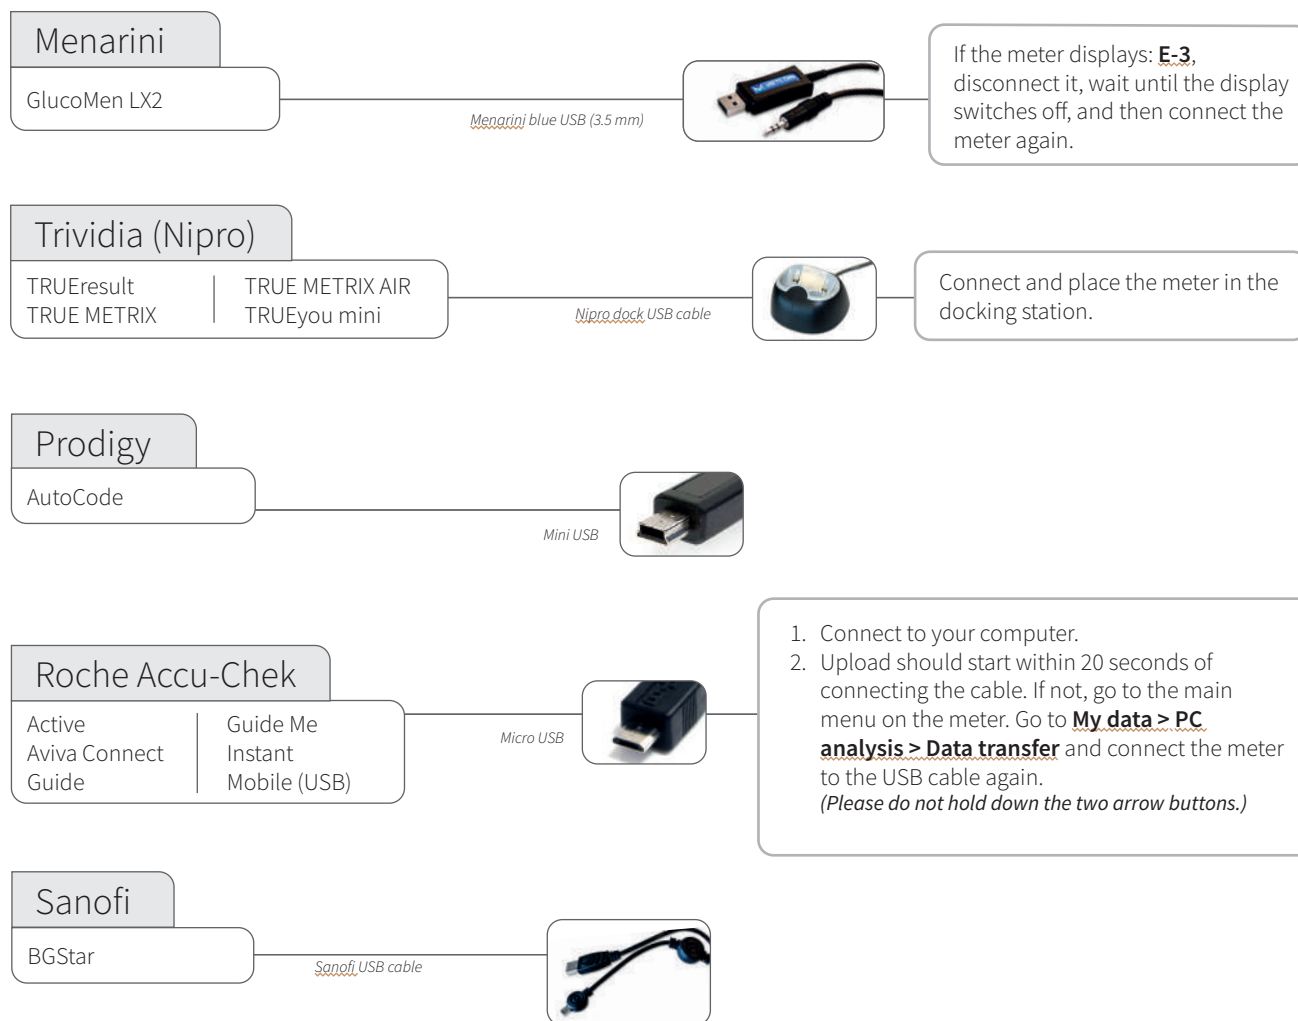


Blood glucose meters – with infrared connection

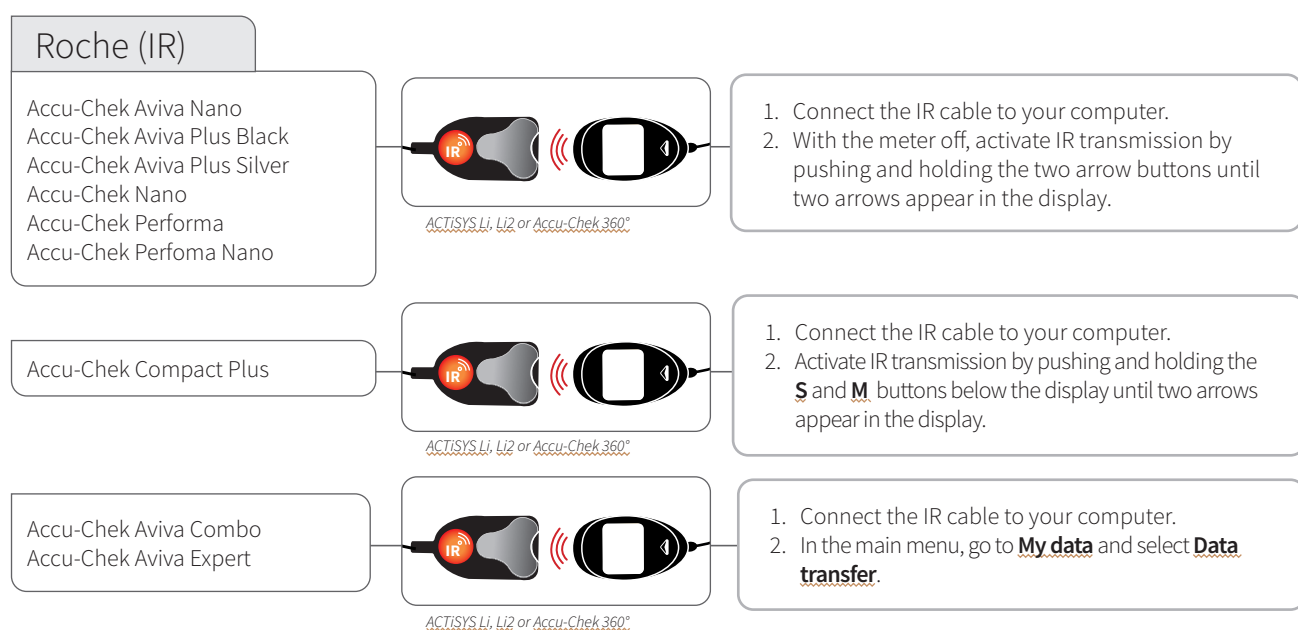



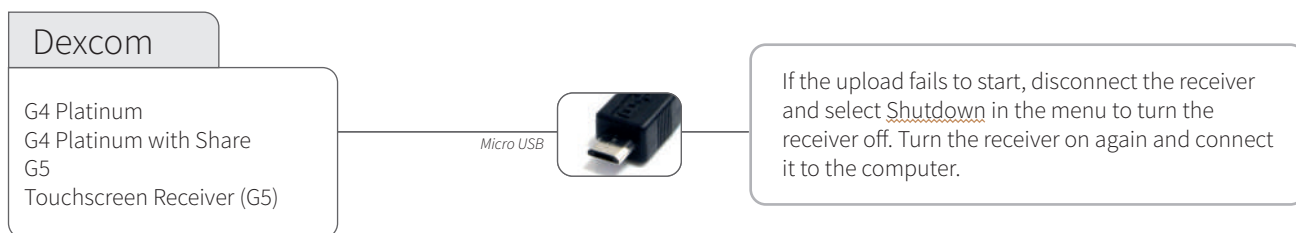

CGMs – connected via USB cable

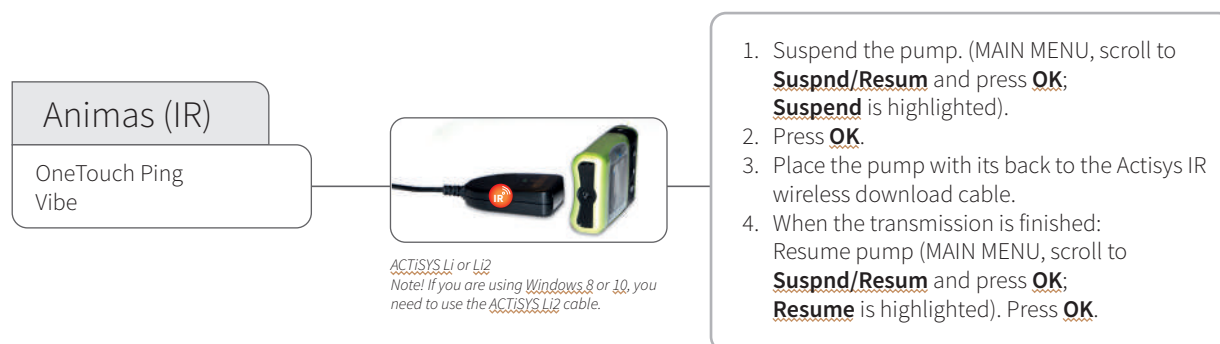

Insulin pumps – with infrared connection



Compatible infrared cables


<p><u>ACTiSYS – Li cable</u></p>  <p>Compatible operating systems: <u>macOS X: 10.14–11.0</u> <u>Windows: N/A</u></p>	<p><u>ACTiSYS – Li2 cable</u></p>  <p>Compatible operating systems: <u>macOS X: 10.14–11.0</u> <u>Windows: 8, 10</u></p>	<p><u>Accu-Chek – 360° cable (Realtyme)</u></p>  <p>Compatible operating systems: <u>macOS X: 10.14–11.0</u> <u>Windows: 8, 10</u></p>	<p><u>Roche Accu-Chek Smart Pix 2 cable</u></p>  <p>Compatible operating systems: <u>macOS X: 10.14–11.0</u> <u>Windows: 8, 10</u></p>
---	--	---	--



Need a cable?

Please contact the manufacturer of your specific diabetes device.

Insulin pumps – connected via USB cable

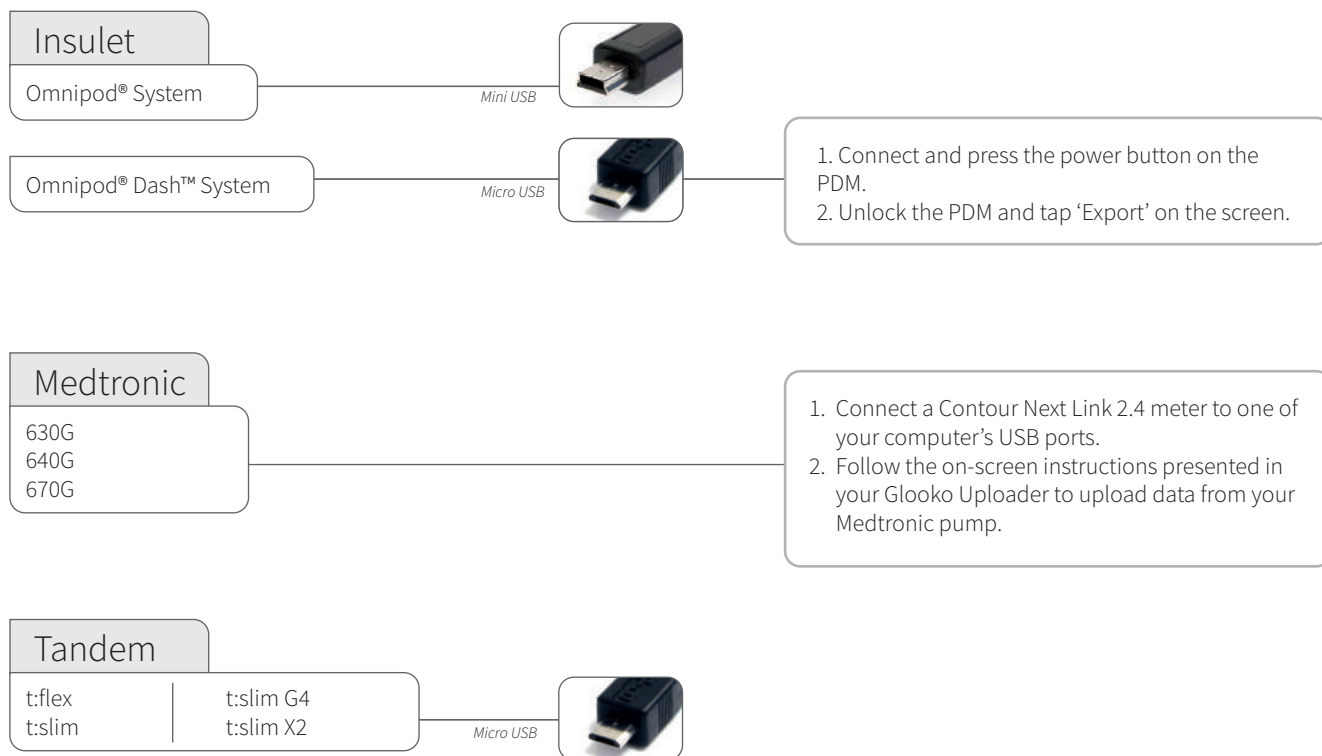

Insulin pumps – connected via infrared cables

Compatible infrared cables


*Roche Accu-Chek
Smart Pix cable*



*Roche Accu-Chek
Smart Pix 2 cable*



Roche
Accu-Chek Aviva Insight
Accu-Chek Performa Insight



Smart Pix 2

Note! Connect the pump handset to Smart Pix 2 using a micro USB cable.

1. Connect the Smart Pix 2 cable to your computer and wait for the blue indicator on Smart Pix 2 to start flashing slowly.
2. Connect the handset to Smart Pix 2 using a micro USB cable.
3. In the handset menu select **Connect to PC** and press **OK**.
4. Ensure that the pump is within range of the handset.
5. The blue indicator on Smart Pix 2 is on while data is being transmitted from the device to Smart Pix 2.
6. The blue indicator turns itself off and both Smart Pix 2 and the device emit a sound to signal that data is being transmitted from Smart Pix 2 to Glooko Uploader. Do not disconnect Smart Pix 2 yet!
7. Wait for Glooko Uploader to confirm the upload was successful.

For more information on Glooko, please contact us on **1300 851 056** or at **diabetes@amsl.com.au**

amsldiabetes.com.au    

AMSL is a subsidiary of Dexcom. PR-100-599 June 2022

